

SUPERVISOR TEST

WASHINGTON COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106406




Date: 11/18/2019

OPERATOR NAME:  
CORY L HURLBURT  
Permit #: 37017  
Operator Agency/Dept: WASHINGTON CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:42
INTERNAL STANDARD	VERIFIED	12:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:43
BLANK TEST	0.00	12:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:44
BLANK TEST	0.00	12:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:45
BLANK TEST	0.00	12:46

CG # 257

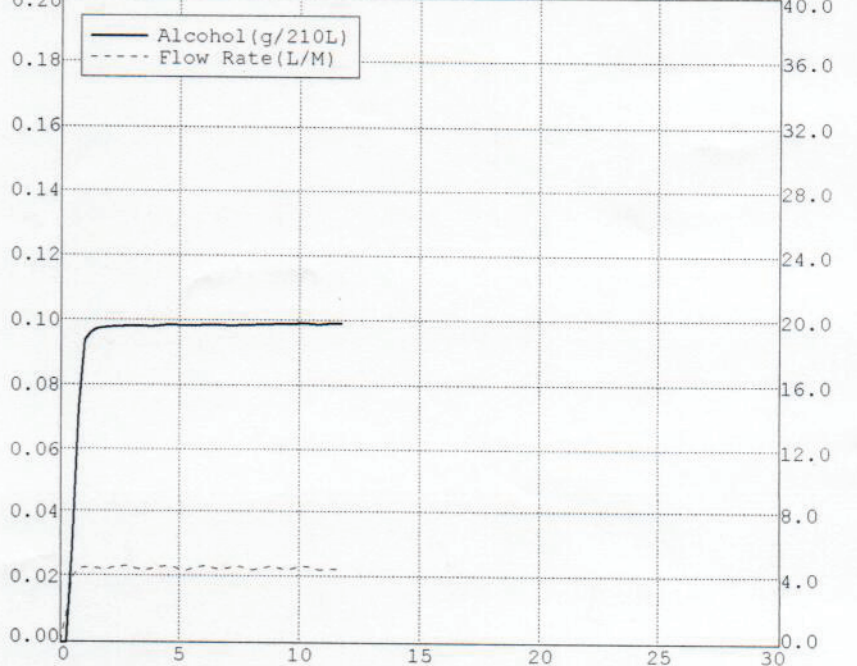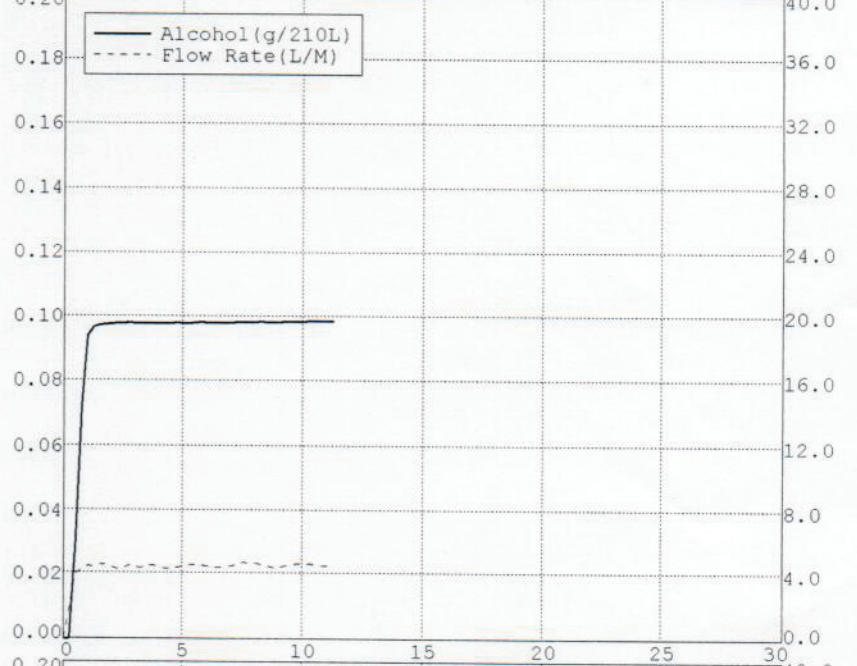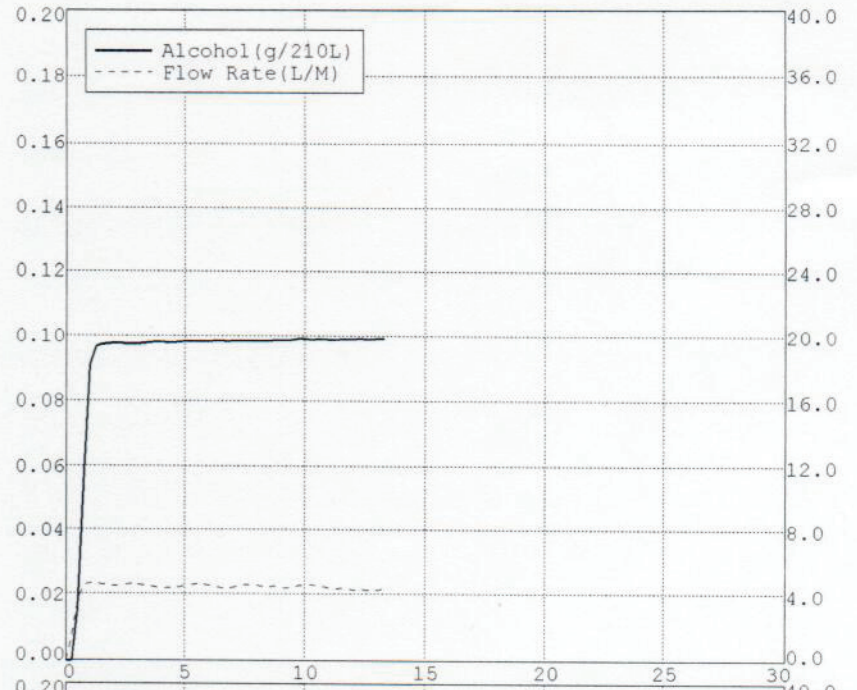



SUPERVISOR TEST

WASHINGTON COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106406

Date: 11/18/2019

OPERATOR NAME:  
CORBET W SULLIVAN  
Permit #: 45898  
Operator Agency/Dept: WASHINGTON CO. SO  
Reference Standard #: 19180

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:45
INTERNAL STANDARD	VERIFIED	21:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:45
BLANK TEST	0.00	21:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:47
BLANK TEST	0.00	21:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:48
BLANK TEST	0.00	21:49

CS #623

