

SUPERVISOR TEST




WASHINGTON CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 100284

Date: 06/17/2019

OPERATOR NAME:  
ROBERT J SULLIVAN  
Permit #: 34106  
Operator Agency/Dept: WASHINGTON CO. SO  
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:20
INTERNAL STANDARD	VERIFIED	21:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:20
BLANK TEST	0.00	21:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:21
BLANK TEST	0.00	21:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	21:22
BLANK TEST	0.00	21:23

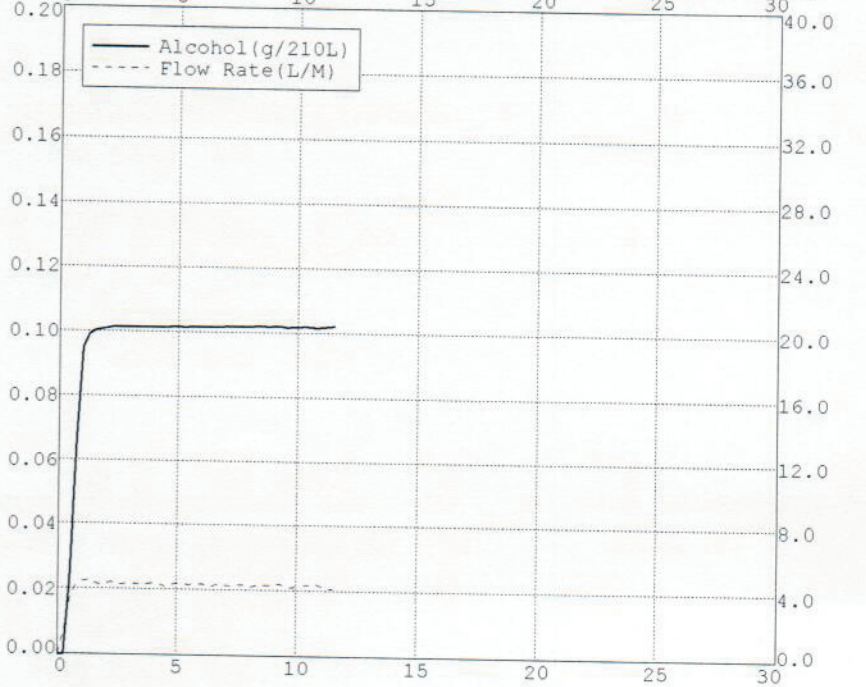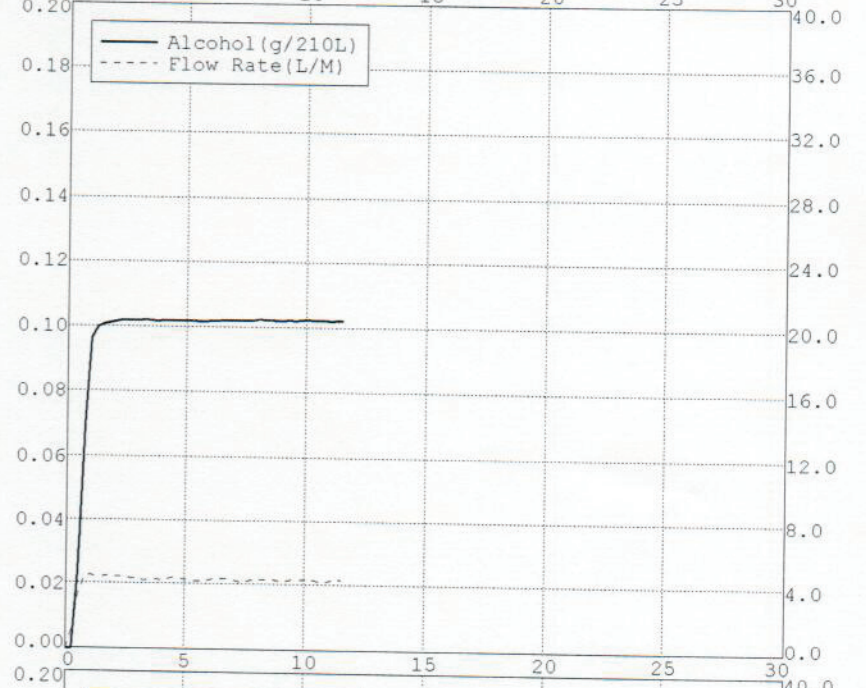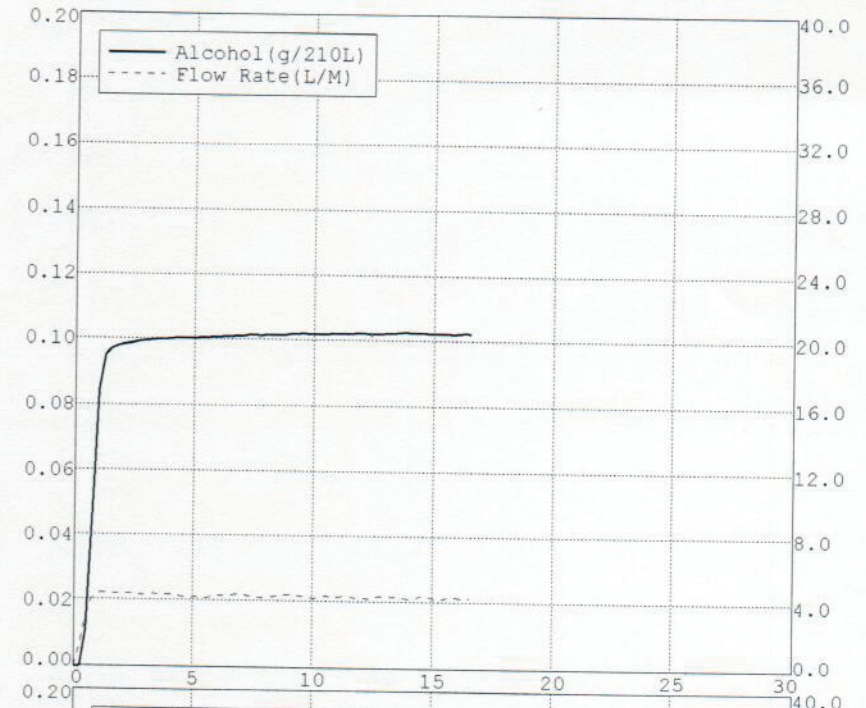

*RS* 698