

SUPERVISOR TEST




WASHINGTON CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 100284

Date: 08/26/2019

OPERATOR NAME:
ROBERT J SULLIVAN
Permit #: 34106
Operator Agency/Dept: WASHINGTON CO. SO
Reference Standard #: 19130

Nominal = 0.10 g/210L

BLANK TEST	0.00	06:12
INTERNAL STANDARD	VERIFIED	06:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:13
BLANK TEST	0.00	06:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:14
BLANK TEST	0.00	06:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	06:15
BLANK TEST	0.00	06:16

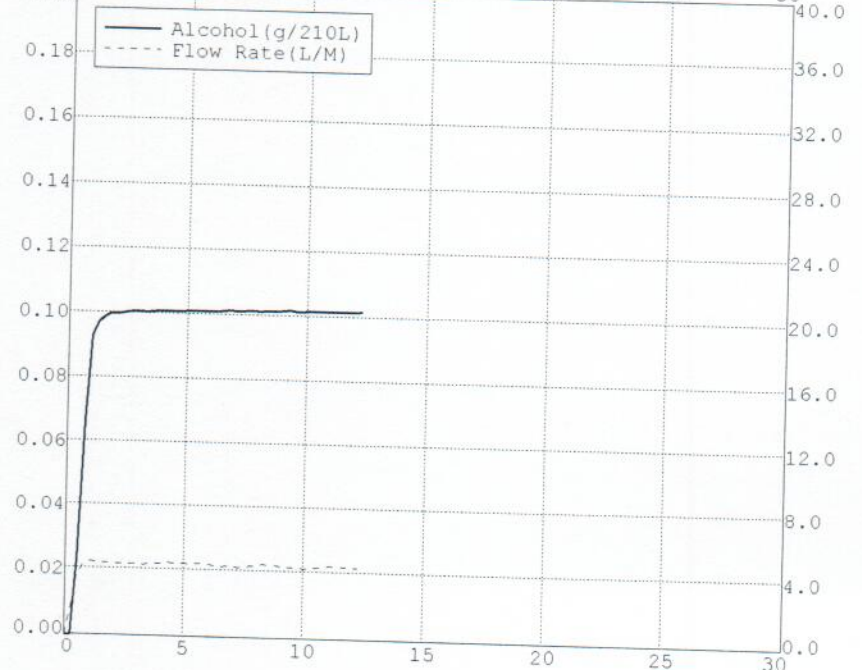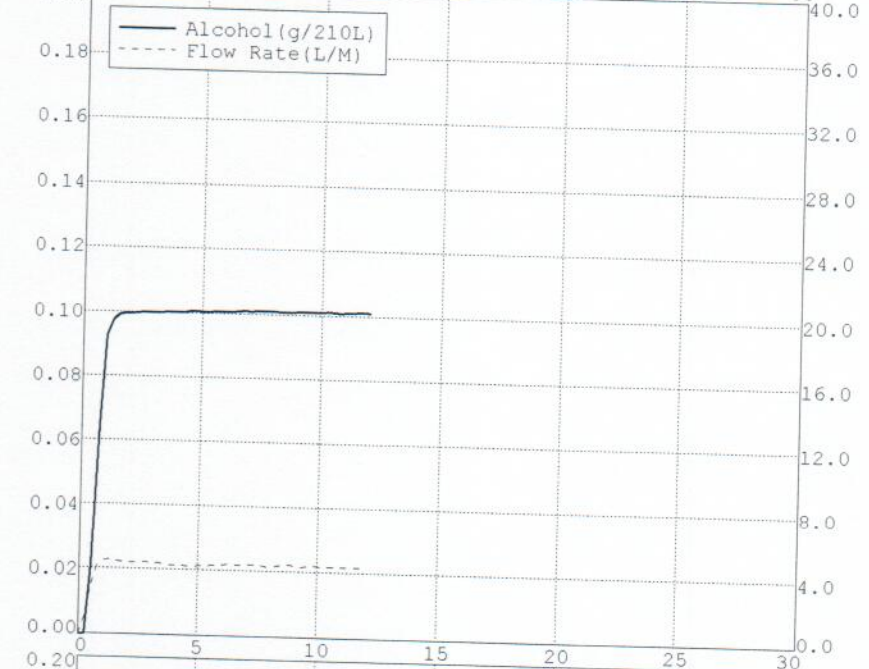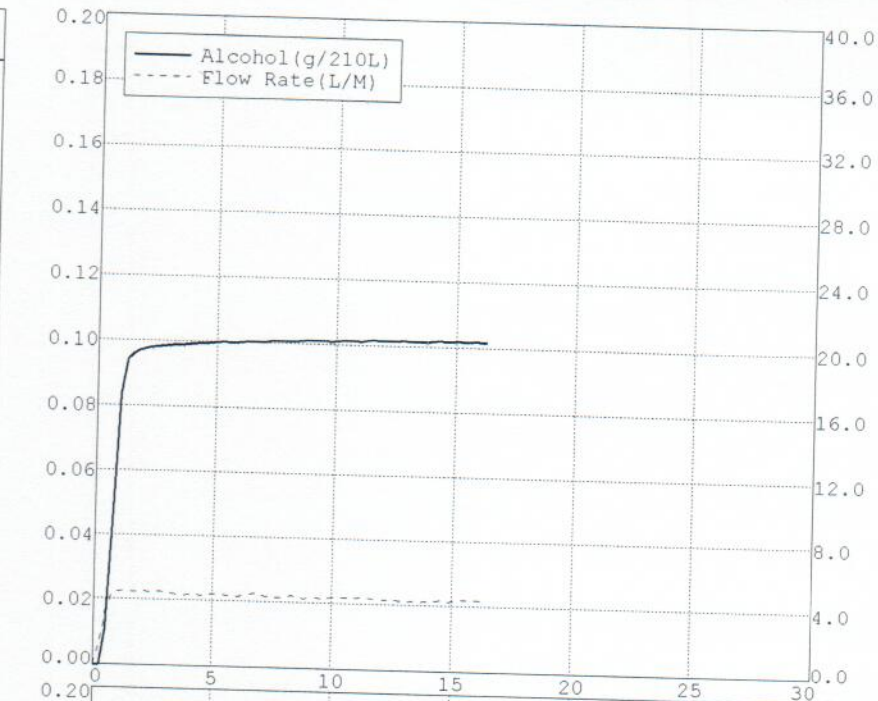

RL 699