

SUPERVISOR TEST




WASHINGTON CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 100284

Date: 07/29/2019

OPERATOR NAME:
ROBERT J SULLIVAN
Permit #: 34106
Operator Agency/Dept: WASHINGTON CO. SO
Reference Standard #: 19090

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:53
INTERNAL STANDARD	VERIFIED	00:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:54
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:55
BLANK TEST	0.00	00:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:56
BLANK TEST	0.00	00:57

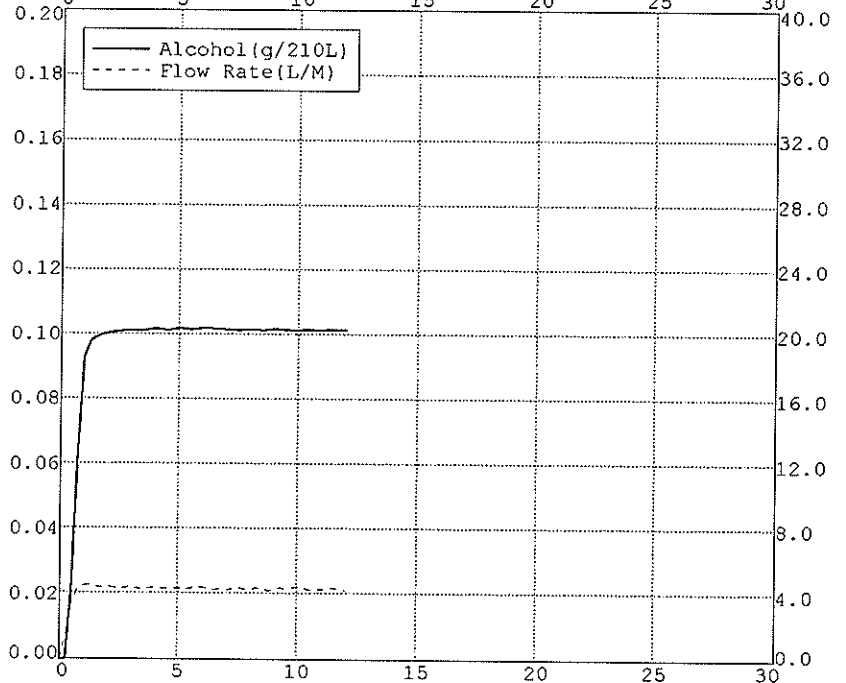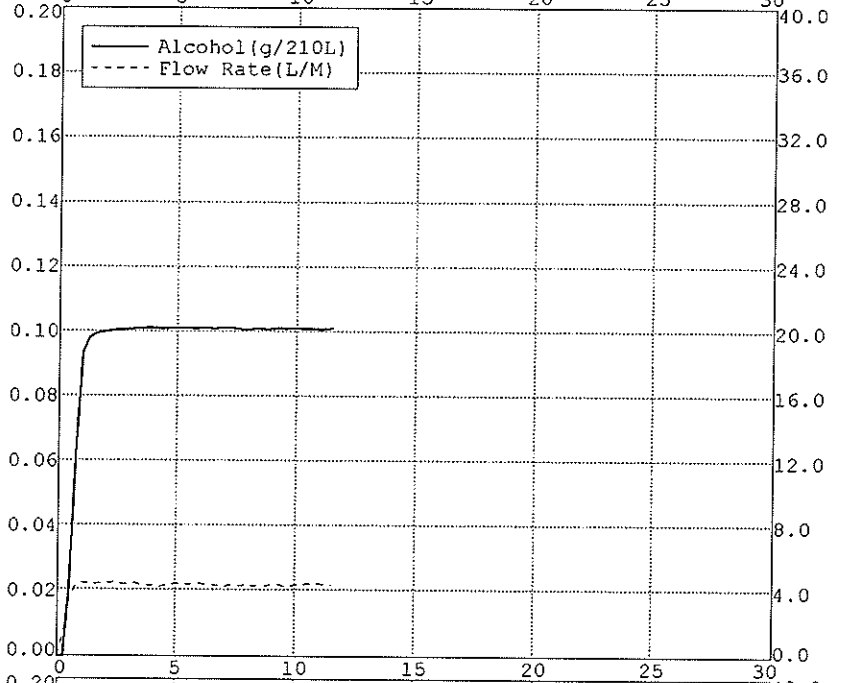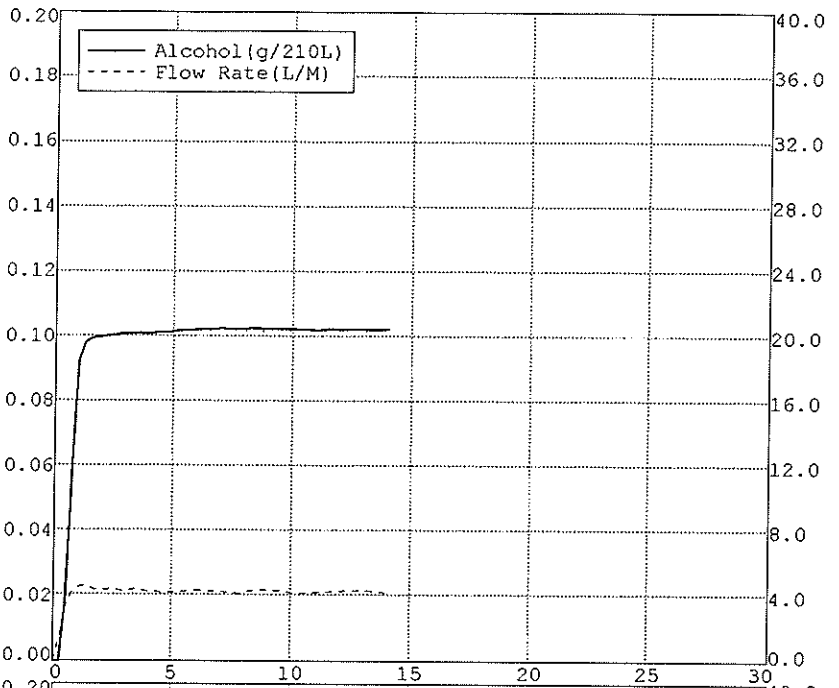

RS 698