

SUPERVISOR TEST




WASHINGTON CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 100284

Date: 02/10/2020

OPERATOR NAME:
ROBERT J SULLIVAN
Permit #: 34106
Operator Agency/Dept: WASHINGTON CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 07:17 |
| INTERNAL STANDARD | VERIFIED | 07:17 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 07:17 |
| BLANK TEST | 0.00 | 07:18 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 07:19 |
| BLANK TEST | 0.00 | 07:19 |
| REFERENCE STANDARD TEMP | 34.00c | |
| REFERENCE STANDARD | 0.10 | 07:20 |
| BLANK TEST | 0.00 | 07:21 |

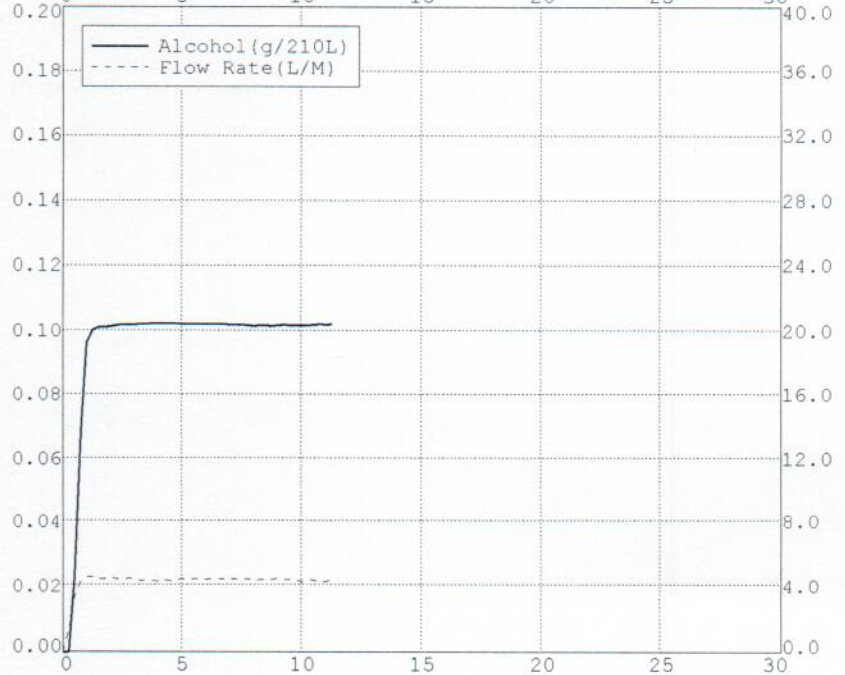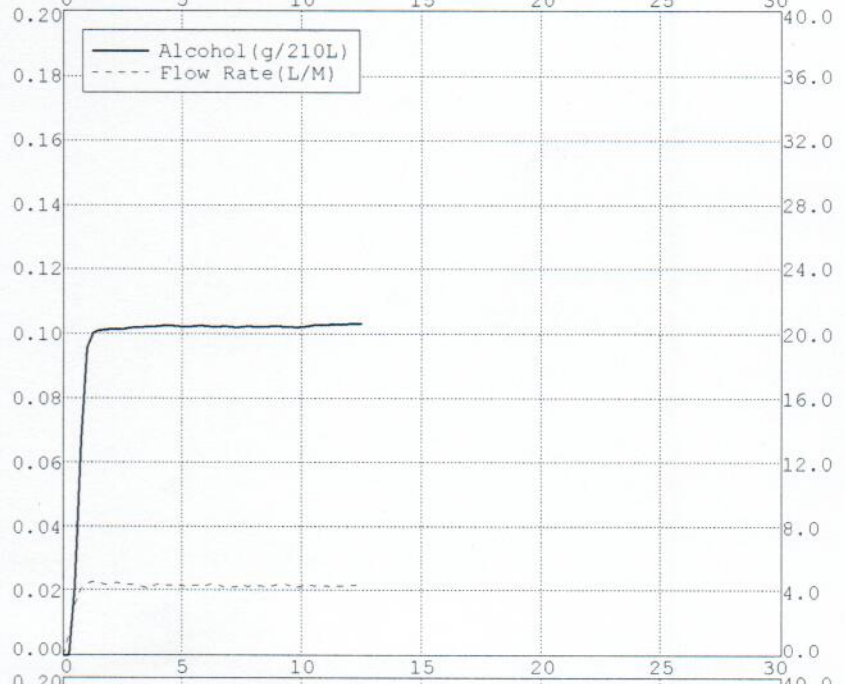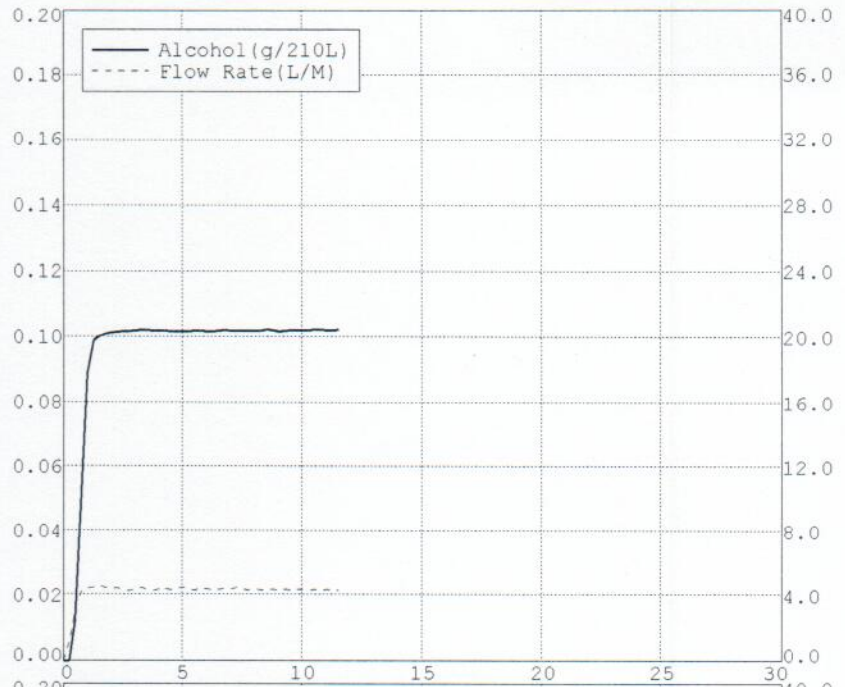

Handwritten signature
698