

SOLUTION CHANGE




HUDSON FALLS
 VILLAGE POLICE DEPT.
 DATAMASTER dmt: 102408

Date: 07/01/2020

OPERATOR NAME:
 BRAD M LYON
 Permit #: 44978
 Operator Agency/Dept: HUDSON FALLS VIL. PD
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:22
INTERNAL STANDARD	VERIFIED	07:22
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	07:22
BLANK TEST	0.00	07:23
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	07:23
BLANK TEST	0.00	07:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:24
BLANK TEST	0.00	07:25

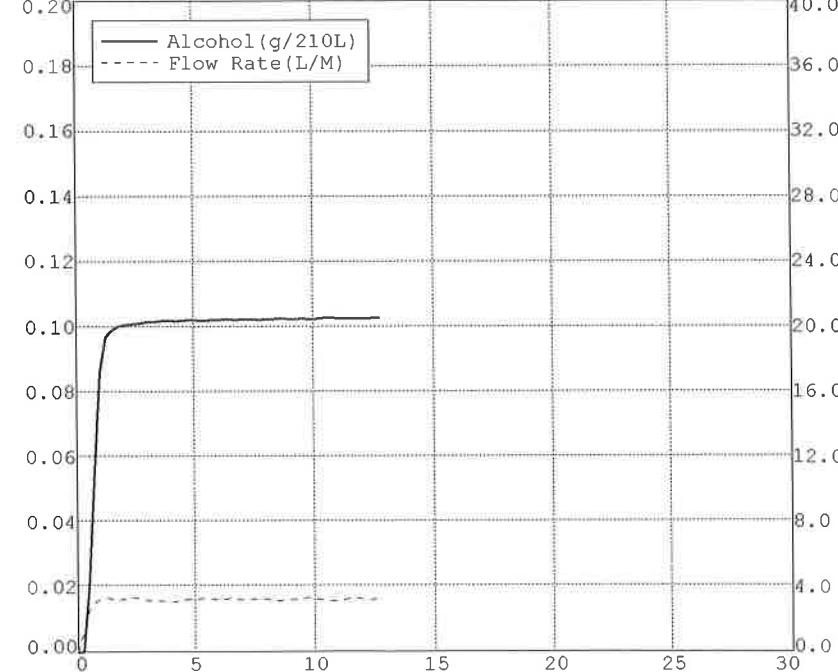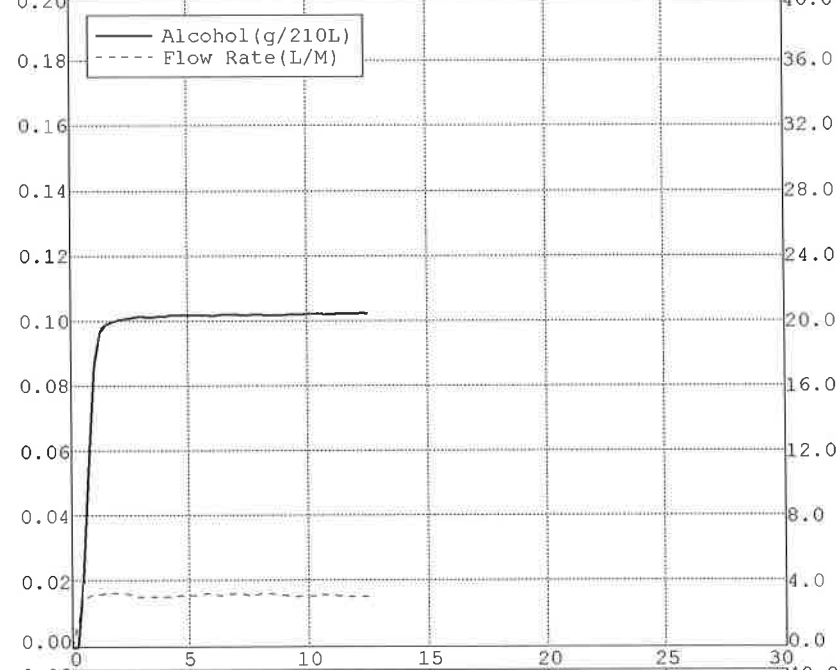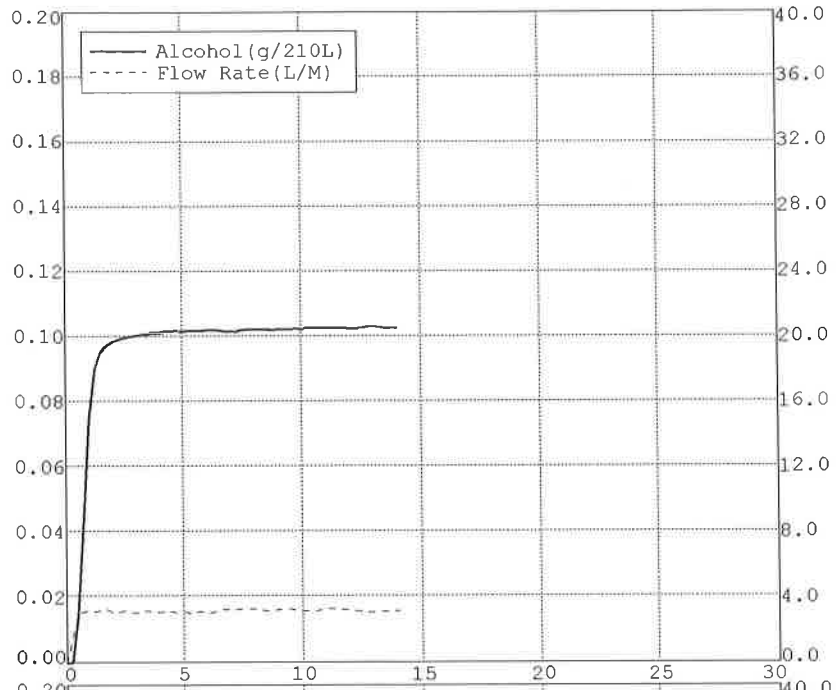

SUPERVISOR TEST

HUDSON FALLS
VILLAGE POLICE DEPT.
DATAMASTER dmt: 102408

Date: 07/01/2020

OPERATOR NAME:
BRAD M LYON
Permit #: 44978
Operator Agency/Dept: HUDSON FALLS VIL. PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:03
INTERNAL STANDARD	VERIFIED	07:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.10	07:03
BLANK TEST	0.00	07:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:04
BLANK TEST	0.00	07:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:06
BLANK TEST	0.00	07:06

