

SUPERVISOR TEST




CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 01/04/2021

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:17
INTERNAL STANDARD	VERIFIED	07:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:17
BLANK TEST	0.00	07:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:18
BLANK TEST	0.00	07:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:19
BLANK TEST	0.00	07:20

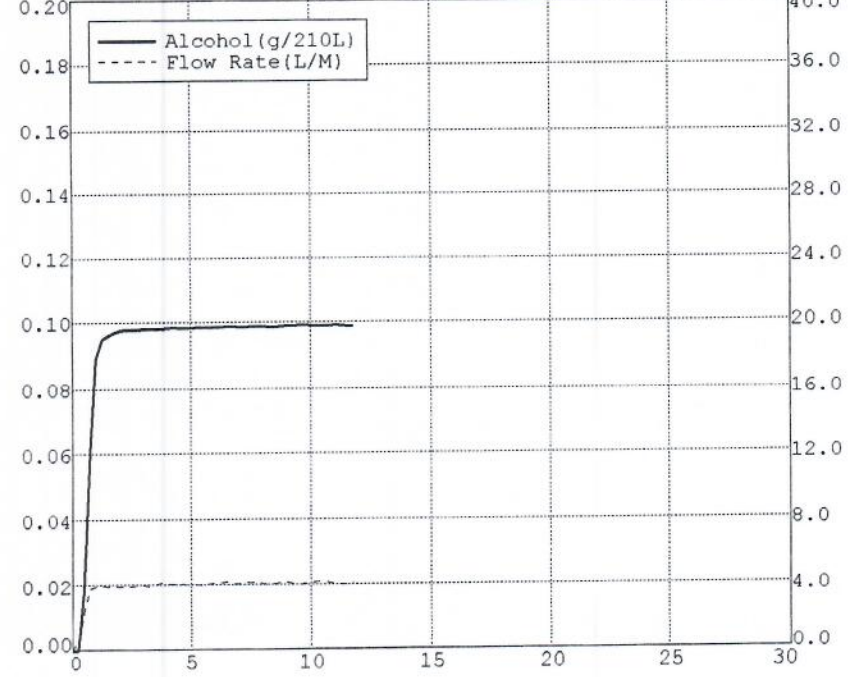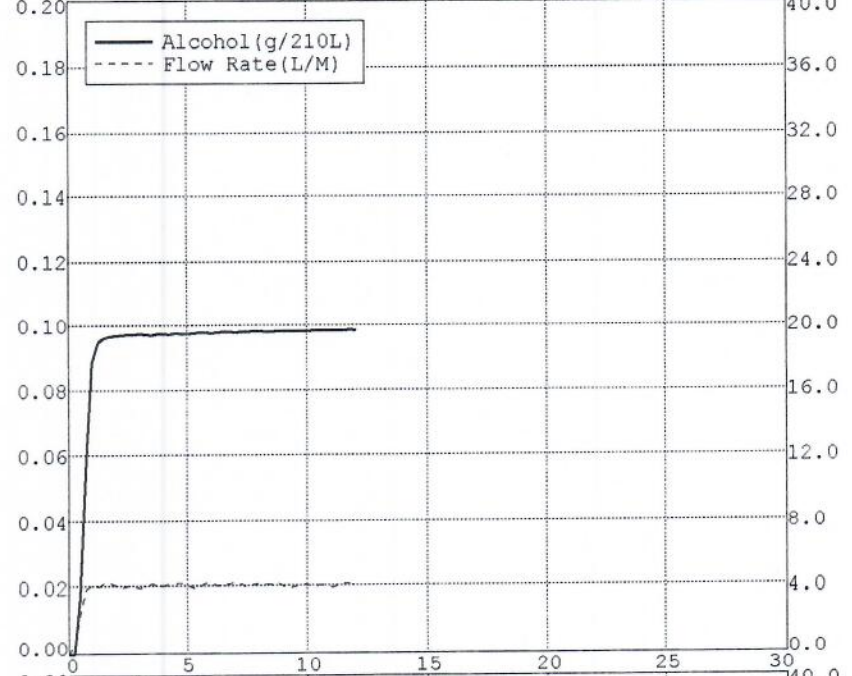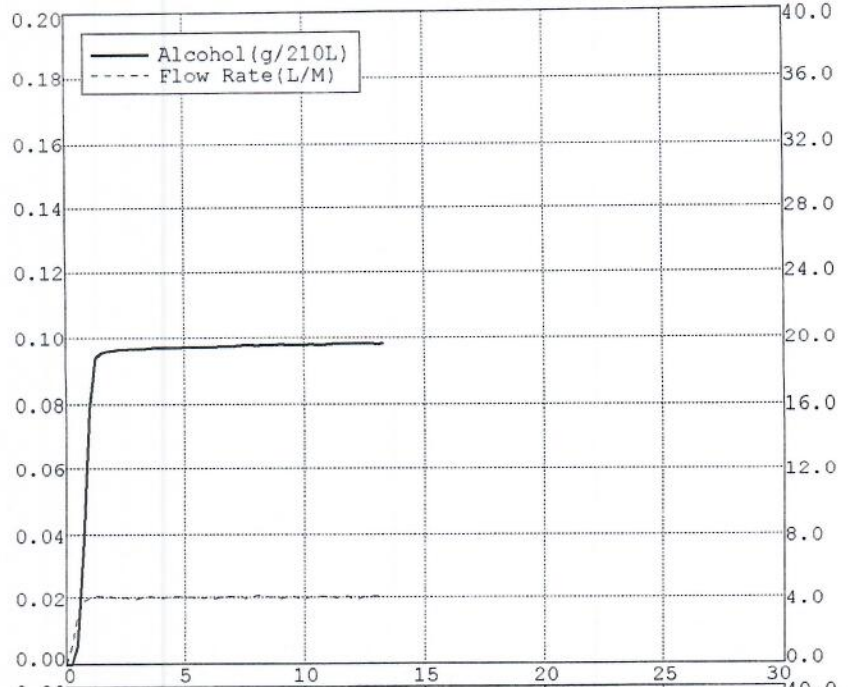

SOLUTION CHANGE

CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 12/30/2020

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:14
INTERNAL STANDARD	VERIFIED	15:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:14
BLANK TEST	0.00	15:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:15
BLANK TEST	0.00	15:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:17
BLANK TEST	0.00	15:17

