

SUPERVISOR TEST




CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 04/06/2021

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:12
INTERNAL STANDARD	VERIFIED	07:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:13
BLANK TEST	0.00	07:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:14
BLANK TEST	0.00	07:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:15
BLANK TEST	0.00	07:16

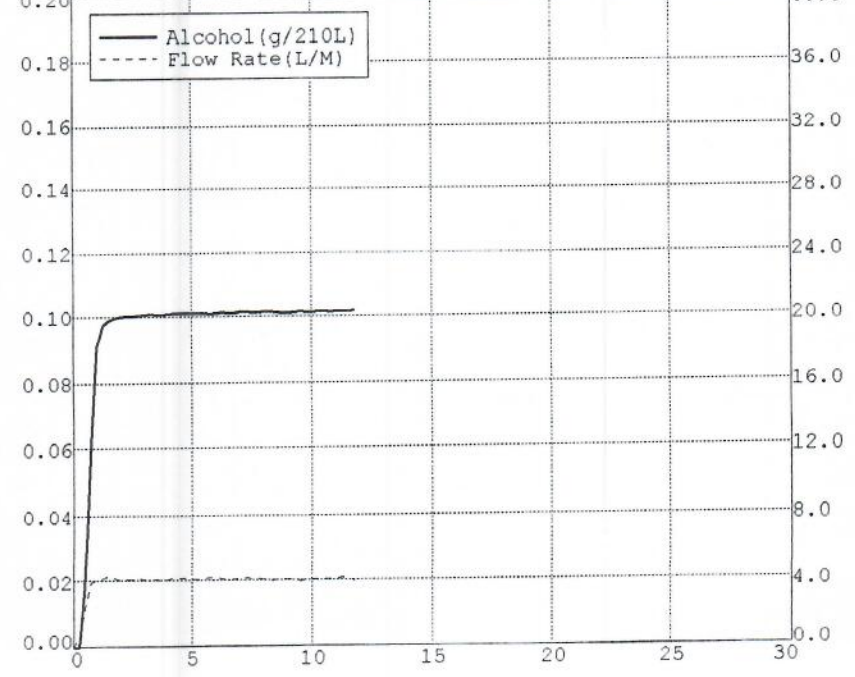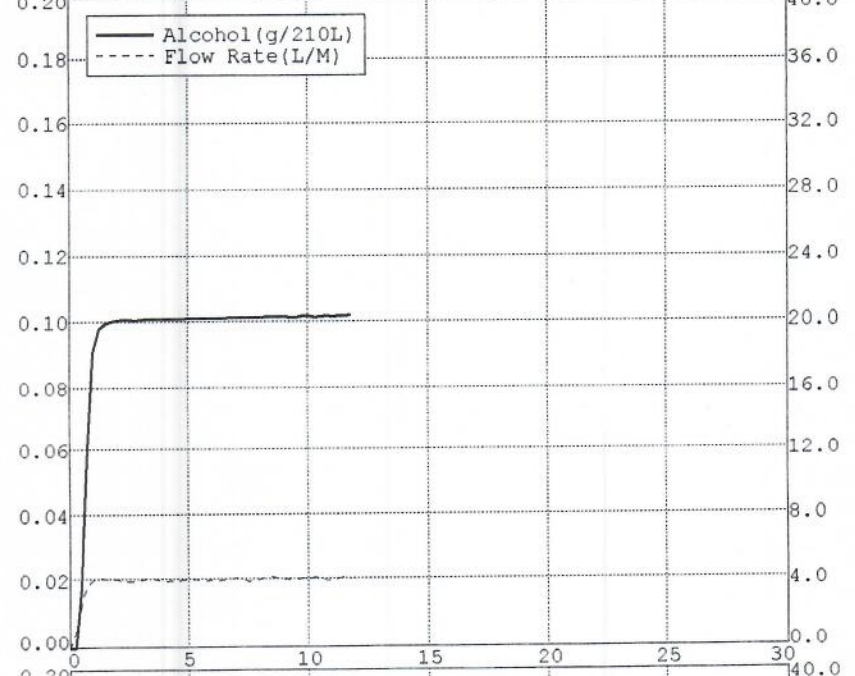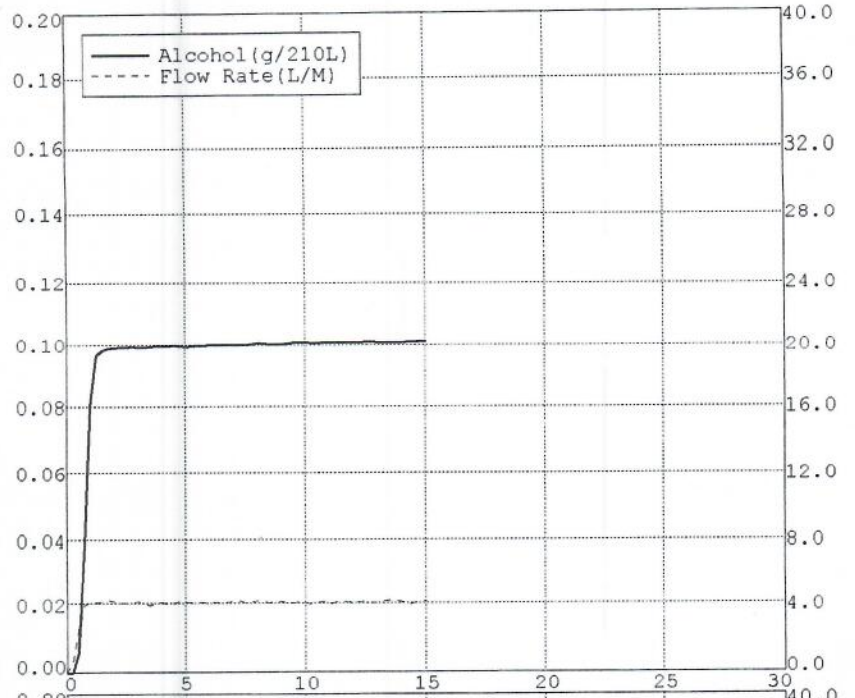

SOLUTION CHANGE

CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 04/02/2021

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:01
INTERNAL STANDARD	VERIFIED	11:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:01
BLANK TEST	0.00	11:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:02
BLANK TEST	0.00	11:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:03
BLANK TEST	0.00	11:04

