

SOLUTION CHANGE



CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 05/03/2021

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:14
INTERNAL STANDARD	VERIFIED	10:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:15
BLANK TEST	0.00	10:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:16
BLANK TEST	0.00	10:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:17
BLANK TEST	0.00	10:18

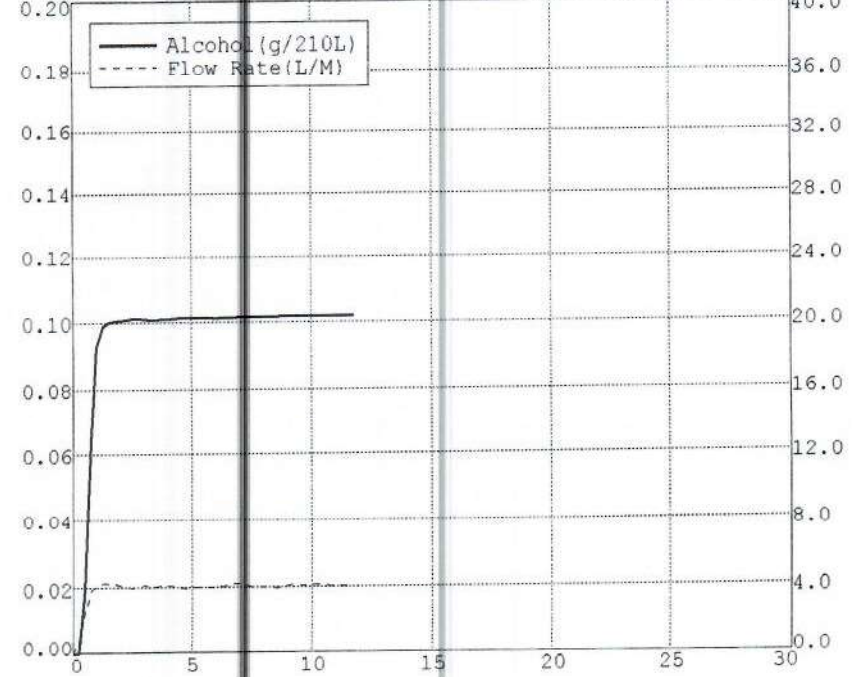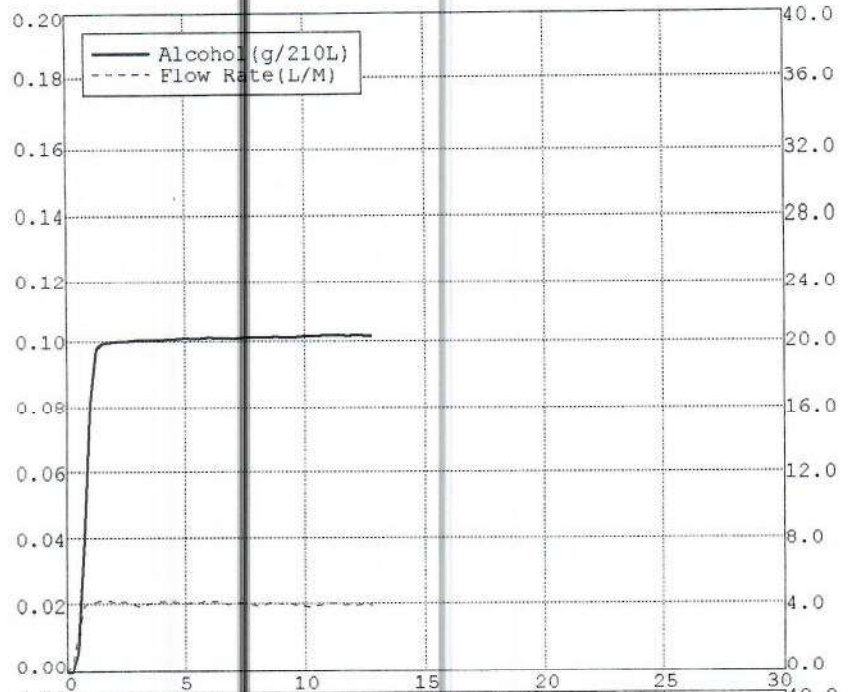

SUPERVISOR TEST

CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 04/26/2021

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:20
INTERNAL STANDARD	VERIFIED	07:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:21
BLANK TEST	0.00	07:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:22
BLANK TEST	0.00	07:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:23
BLANK TEST	0.00	07:24

