

SUPERVISOR TEST



-----  
 CAMBRIDGE VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 126706  
 -----

Date: 06/28/2021

OPERATOR NAME:  
 ROBERT M DANKO  
 Permit #: 39105  
 Operator Agency/Dept: CAMBRIDGE VILL. PD  
 Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:09
INTERNAL STANDARD	VERIFIED	08:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:09
BLANK TEST	0.00	08:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:10
BLANK TEST	0.00	08:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:12
BLANK TEST	0.00	08:12

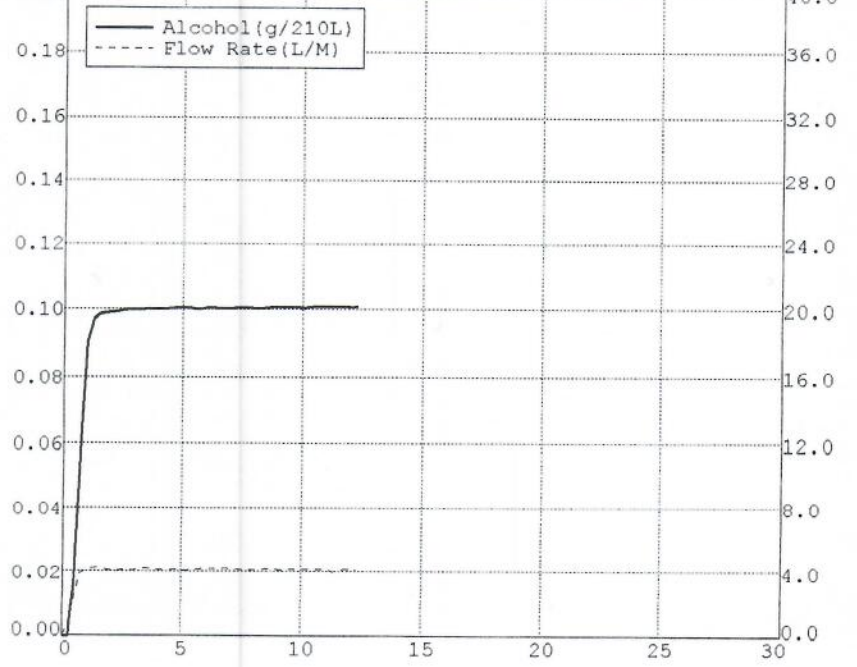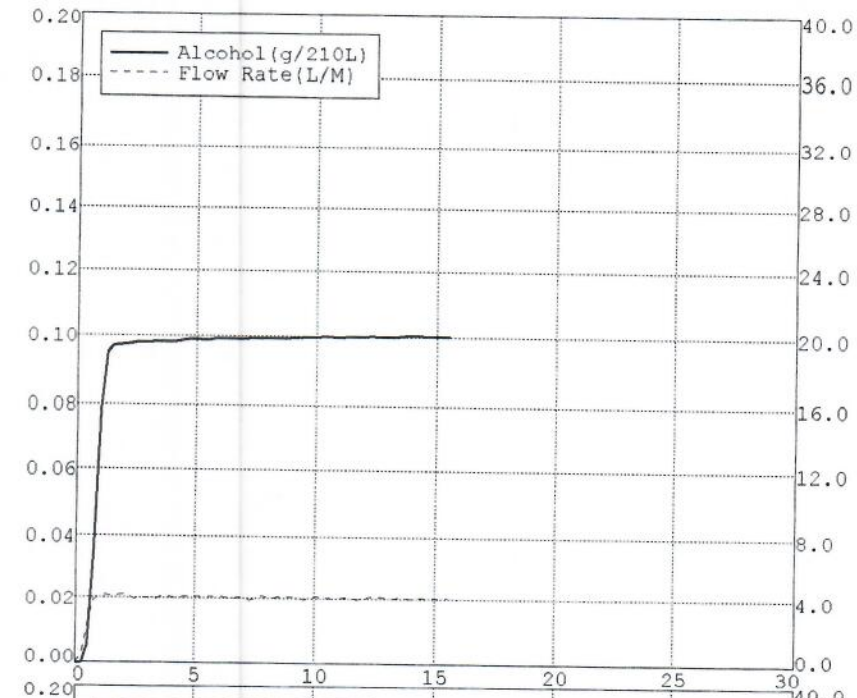

SOLUTION CHANGE

-----  
 CAMBRIDGE VILLAGE  
 POLICE DEPT  
 DATAMASTER dmt: 126706  
 -----

Date: 07/01/2021

OPERATOR NAME:  
 ROBERT M DANKO  
 Permit #: 39105  
 Operator Agency/Dept: CAMBRIDGE VILL. PD  
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:05
INTERNAL STANDARD	VERIFIED	14:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:06
BLANK TEST	0.00	14:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:07
BLANK TEST	0.00	14:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:08
BLANK TEST	0.00	14:09

