

SUPERVISOR TEST




CAMBRIDGE VILLAGE
POLICE DEPT
DATAMASTER dmt: 126706

Date: 08/08/2022

OPERATOR NAME:
ROBERT M DANKO
Permit #: 39105
Operator Agency/Dept: CAMBRIDGE VILL. PD
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:39
INTERNAL STANDARD	VERIFIED	08:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:40
BLANK TEST	0.00	08:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	08:41
BLANK TEST	0.00	08:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	08:42
BLANK TEST	0.00	08:43

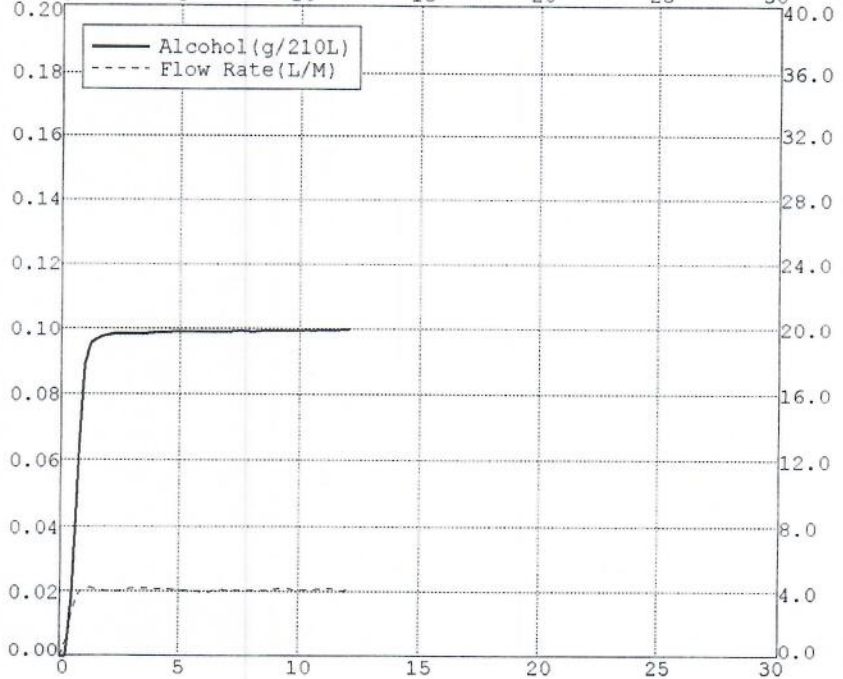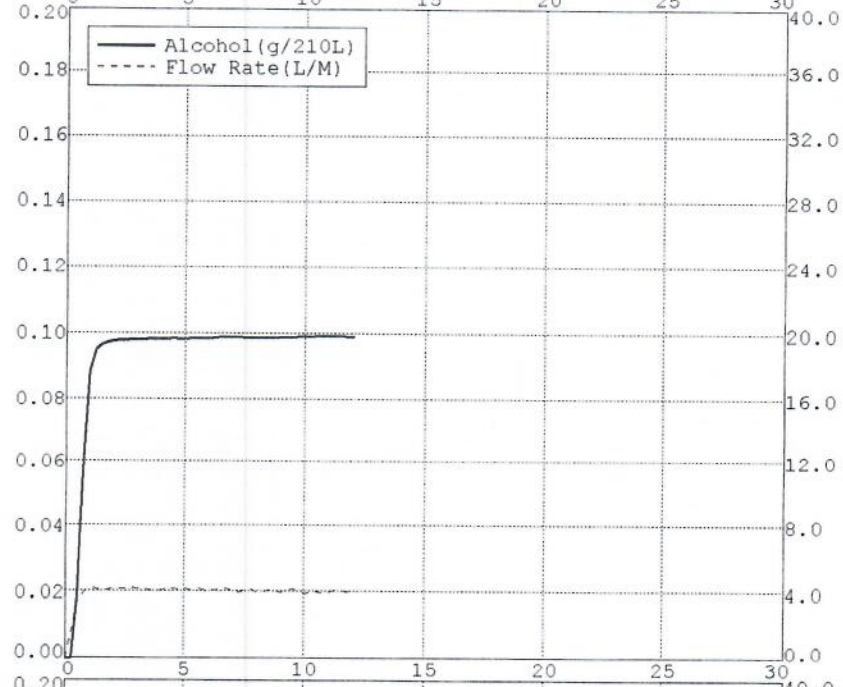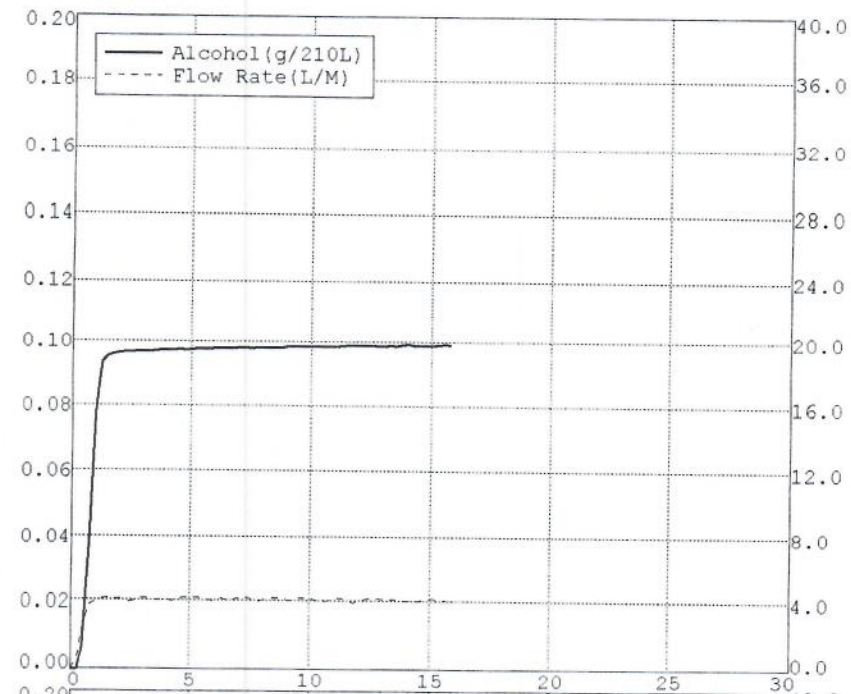

SUPERVISOR TEST

 CAMBRIDGE VILLAGE
 POLICE DEPT
 DATAMASTER dmt: 126706

Date: 08/16/2022

OPERATOR NAME:
 ROBERT M DANKO
 Permit #: 39105
 Operator Agency/Dept: CAMBRIDGE VILL. PD
 Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:07
INTERNAL STANDARD	VERIFIED	07:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:08
BLANK TEST	0.00	07:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	07:09
BLANK TEST	0.00	07:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	07:10
BLANK TEST	0.00	07:11

